

# ILNAS

Institut luxembourgeois de la normalisation  
de l'accréditation, de la sécurité et qualité  
des produits et services


## ILNAS-EN ISO 80601-2-12:2020

### **Medical electrical equipment - Part 2-12: Particular requirements for basic safety and essential performance of critical care ventilators (ISO**

Medizinische elektrische Geräte - Teil  
2-12: Besondere Festlegungen für die  
Sicherheit einschließlich der  
wesentlichen Leistungsmerkmale von

Appareils électromédicaux - Partie 2-12:  
Exigences particulières relatives à la  
sécurité de base et aux performances  
essentielles des ventilateurs pulmonaires

03/2020

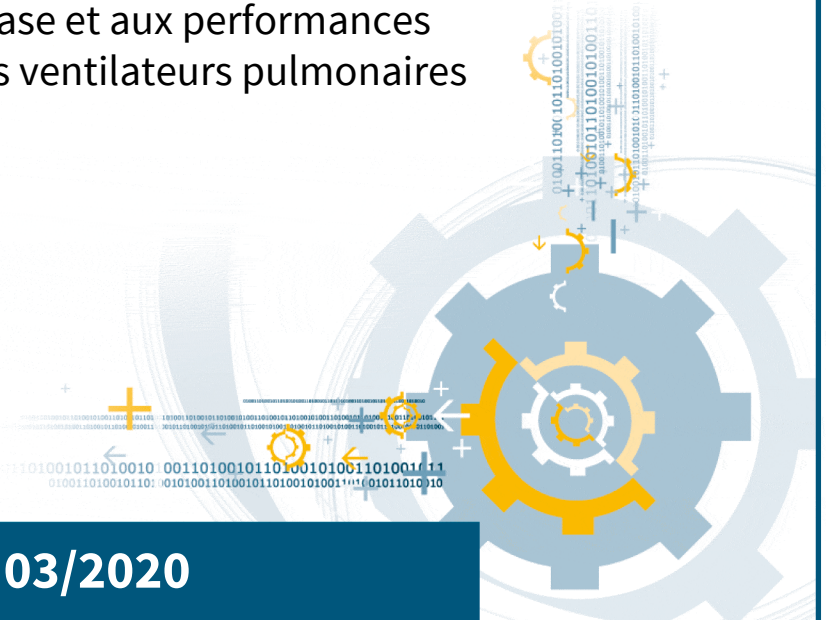

## National Foreword

This European Standard EN ISO 80601-2-12:2020 was adopted as Luxembourgish Standard ILNAS-EN ISO 80601-2-12:2020.

Every interested party, which is member of an organization based in Luxembourg, can participate for FREE in the development of Luxembourgish (ILNAS), European (CEN, CENELEC) and International (ISO, IEC) standards:

- Participate in the design of standards
- Foresee future developments
- Participate in technical committee meetings

<https://portail-qualite.public.lu/fr/normes-normalisation/participer-normalisation.html>

### **THIS PUBLICATION IS COPYRIGHT PROTECTED**

Nothing from this publication may be reproduced or utilized in any form or by any mean - electronic, mechanical, photocopying or any other data carries without prior permission!

ILNAS-EN ISO 80601-2-12:2020

EUROPEAN STANDARD **EN ISO 80601-2-12**

NORME EUROPÉENNE

EUROPÄISCHE NORM

March 2020

ICS 11.040.10

Supersedes EN ISO 80601-2-12:2011

English Version

**Medical electrical equipment - Part 2-12: Particular requirements for basic safety and essential performance of critical care ventilators (ISO 80601-2-12:2020)**

Appareils électromédicaux - Partie 2-12: Exigences particulières relatives à la sécurité de base et aux performances essentielles des ventilateurs pulmonaires pour utilisation en soins intensifs (ISO 80601-2-12:2020)

Medizinische elektrische Geräte - Teil 2-12: Besondere Festlegungen für die Sicherheit einschließlich der wesentlichen Leistungsmerkmale von Beatmungsgeräten für die Intensivpflege (ISO 80601-2-12:2020)

This European Standard was approved by CEN on 12 November 2019.

CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration. Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the CEN-CENELEC Management Centre or to any CEN member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the CEN-CENELEC Management Centre has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Bulgaria, Croatia, Cyprus, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Republic of North Macedonia, Romania, Serbia, Slovakia, Slovenia, Spain, Sweden, Switzerland, Turkey and United Kingdom.



EUROPEAN COMMITTEE FOR STANDARDIZATION  
COMITÉ EUROPÉEN DE NORMALISATION  
EUROPÄISCHES KOMITEE FÜR NORMUNG

**CEN-CENELEC Management Centre: Rue de la Science 23, B-1040 Brussels**

**Contents**

Page

**European foreword..... 3**

ILNAS-EN ISO 80601-2-12:2020 - Preview only Copy via ILNAS e-Shop

## European foreword

This document (EN ISO 80601-2-12:2020) has been prepared by Technical Committee ISO/TC 121 "Anaesthetic and respiratory equipment" in collaboration with Technical Committee CEN/TC 215 "Respiratory and anaesthetic equipment" the secretariat of which is held by BSI.

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by September 2020, and conflicting national standards shall be withdrawn at the latest by September 2020.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. CEN shall not be held responsible for identifying any or all such patent rights.

This document supersedes EN ISO 80601-2-12:2011.

According to the CEN-CENELEC Internal Regulations, the national standards organizations of the following countries are bound to implement this European Standard: Austria, Belgium, Bulgaria, Croatia, Cyprus, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Republic of North Macedonia, Romania, Serbia, Slovakia, Slovenia, Spain, Sweden, Switzerland, Turkey and the United Kingdom.

## Endorsement notice

The text of ISO 80601-2-12:2020 has been approved by CEN as EN ISO 80601-2-12:2020 without any modification.

---

---

**Medical electrical equipment —**  
**Part 2-12:**  
**Particular requirements for basic**  
**safety and essential performance of**  
**critical care ventilators**

*Appareils électromédicaux —*

*Partie 2-12: Exigences particulières relatives à la sécurité de base  
et aux performances essentielles des ventilateurs pulmonaires pour  
utilisation en soins intensifs*



**COPYRIGHT PROTECTED DOCUMENT**

© ISO 2020

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
CP 401 • Ch. de Blandonnet 8  
CH-1214 Vernier, Geneva  
Phone: +41 22 749 01 11  
Fax: +41 22 749 09 47  
Email: [copyright@iso.org](mailto:copyright@iso.org)  
Website: [www.iso.org](http://www.iso.org)

Published in Switzerland

## Contents

<b>201. 1</b>	<b>Scope, object and related standards</b> .....	<b>1</b>
201. 1.1	* Scope .....	1
201. 1.2	Object.....	2
201. 1.3	Collateral standards .....	3
201. 1.4	Particular standards.....	3
<b>201. 2</b>	<b>Normative references</b> .....	<b>4</b>
<b>201. 3</b>	<b>Terms and definitions</b> .....	<b>7</b>
<b>201. 4</b>	<b>General requirements</b> .....	<b>9</b>
201. 4.3	<i>Essential performance</i> .....	9
201. 4.3.101	* Additional requirements for <i>essential performance</i> .....	9
201. 4.4	Additional requirements for <i>expected service life</i> .....	9
201. 4.6	* <i>ME equipment</i> or <i>ME system</i> parts that contact the <i>patient</i> .....	10
201. 4.11.101	* Additional requirements for pressurized gas input.....	10
201. 4.11.101.1	Overpressure requirement.....	10
201. 4.11.101.2	Compatibility requirement.....	10
<b>201. 5</b>	<b>General requirements for testing of <i>ME equipment</i></b> .....	<b>11</b>
201. 5.101	Additional requirements for general requirements for testing of <i>ME equipment</i> .....	11
201. 5.101.1	<i>Ventilator</i> test conditions .....	11
201. 5.101.2	* Gas flowrate and leakage specifications.....	11
201. 5.101.3	* <i>Ventilator</i> testing errors.....	11
<b>201. 6</b>	<b>Classification of <i>ME equipment</i> and <i>ME systems</i></b> .....	<b>12</b>
<b>201. 7</b>	<b><i>ME equipment</i> identification, marking and documents</b> .....	<b>12</b>
201. 7.2.3	* Consult <i>accompanying documents</i> .....	12
201. 7.2.4.101	Additional requirements for <i>accessories</i> .....	12
201. 7.2.13.101	Additional requirements for physiological effects .....	12
201. 7.2.17.101	Additional requirements for protective packaging.....	12
201. 7.2.18	External gas source.....	13
201. 7.2.101	* Additional requirements for marking on the outside of <i>ME equipment</i> or <i>ME equipment</i> parts .....	13
201. 7.4.3	* Units of measurement.....	14
201. 7.9.1	Additional general requirements .....	14
201. 7.9.2.1.101	Additional general requirements .....	14
201. 7.9.2.2.101	* Additional requirements for warnings and safety notices....	15
201. 7.9.2.8.101	* Additional requirements for start-up <i>procedure</i> .....	16
201. 7.9.2.9.101	* Additional requirements for operating instructions .....	16
201. 7.9.2.12	<i>Cleaning, disinfection, and sterilization</i> .....	17
201. 7.9.2.14.101	* Additional requirements for <i>accessories</i> , supplementary equipment, used material.....	17



201. 7.9.2.16.101	* Additional requirements for reference to the technical description .....	18
201. 7.9.3.1.101	* Additional general requirements .....	18
201. 7.9.3.101	Additional requirements for the technical description .....	18
<b>201. 8</b>	<b>Protection against electrical hazards from ME equipment.....</b>	<b>19</b>
<b>201. 9</b>	<b>Protection against mechanical hazards of ME equipment and ME systems</b>	<b>19</b>
201. 9.6.2.1.101	* Additional requirements for audible acoustic energy.....	19
201. 9.101	* Additional requirements for suction procedures.....	20
<b>201. 10</b>	<b>Protection against unwanted and excessive radiation hazards.....</b>	<b>23</b>
<b>201. 11</b>	<b>Protection against excessive temperatures and other hazards.....</b>	<b>23</b>
201. 11.1.2.2	* Applied parts not intended to supply heat to a patient .....	23
201. 11.6.5.101	* Additional requirements for ingress of water or particulate matter into ME equipment or ME system .....	23
201. 11.6.6	* Cleaning and disinfection of ME equipment or ME system.....	24
201. 11.6.7	Sterilization of ME equipment or ME system .....	24
201. 11.7	Biocompatibility of ME equipment and ME systems .....	24
201. 11.8.101	* Additional requirements for interruption of the power supply/supply mains to ME equipment .....	25
<b>201. 12</b>	<b>Accuracy of controls and instruments and protection against hazardous outputs.....</b>	<b>27</b>
201. 12.1	* Accuracy of controls and instruments .....	27
201. 12.1.101	* Volume-control inflation-type .....	27
201. 12.1.102	* Pressure-control inflation-type .....	31
201. 12.1.103	Other inflation-types.....	34
201. 12.1.104	* Inspiratory volume monitoring .....	35
201. 12.1.105	* Response of the ventilator to an increase in set O <sub>2</sub> concentration .....	35
201. 12.4	Protection against hazardous output.....	37
201. 12.4.101	Oxygen monitor .....	37
201. 12.4.102	* Measurement of airway pressure.....	38
201. 12.4.103	* Measurement of expired volume and low volume alarm conditions .....	39
201. 12.4.103.1	Ventilators intended to provide a tidal volume >50 ml.....	39
201. 12.4.103.2	Ventilators intended to provide a tidal volume ≤50 ml.....	40
201. 12.4.104	* Expiratory end-tidal CO <sub>2</sub> monitoring equipment.....	41
201. 12.4.105	* Maximum limited pressure protection device .....	42
201. 12.4.106	* High airway pressure alarm condition and protection device	42
201. 12.4.107	PEEP alarm conditions .....	43
201. 12.4.108	* Obstruction alarm condition .....	44
201. 12.4.109	* Disconnection alarm condition.....	45
201. 12.4.110	Protection against inadvertent setting of high airway pressure .....	45
201. 12.101	* Protection against accidental or unintentional adjustments	45
<b>201. 13</b>	<b>Hazardous situations and fault conditions for ME equipment .....</b>	<b>46</b>